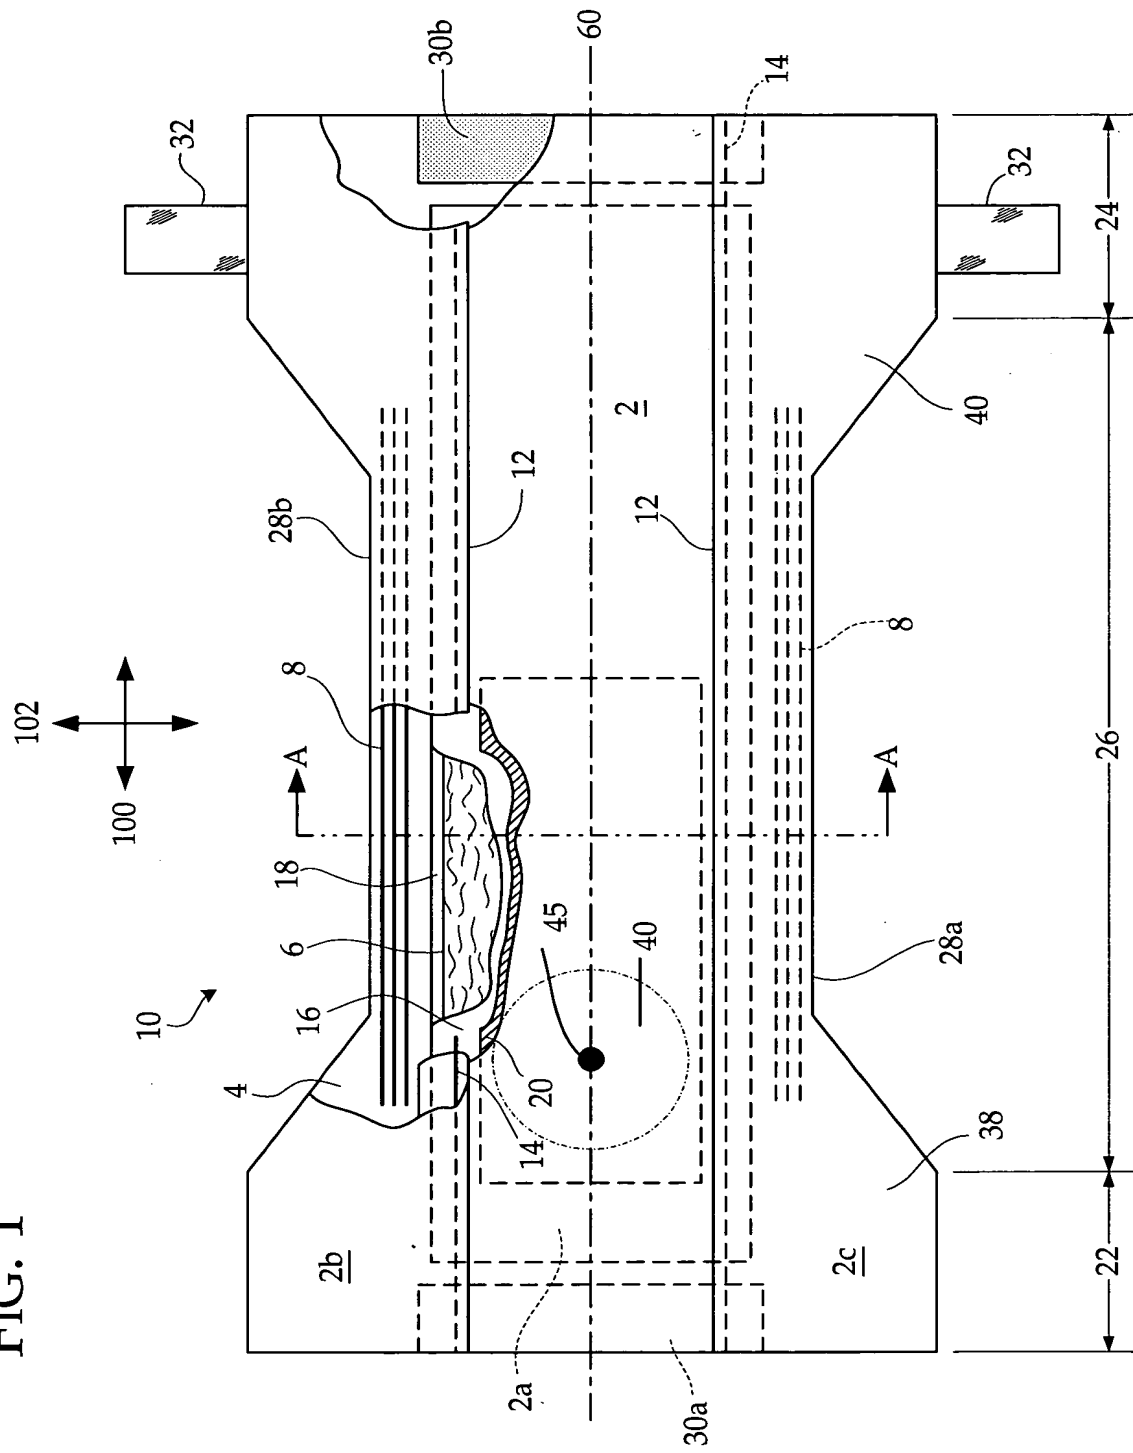


FIG. 1



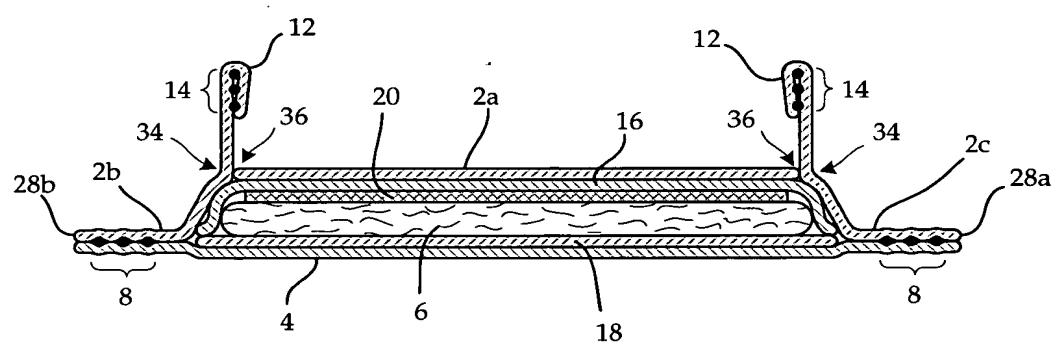
[illegible]

FIG. 3

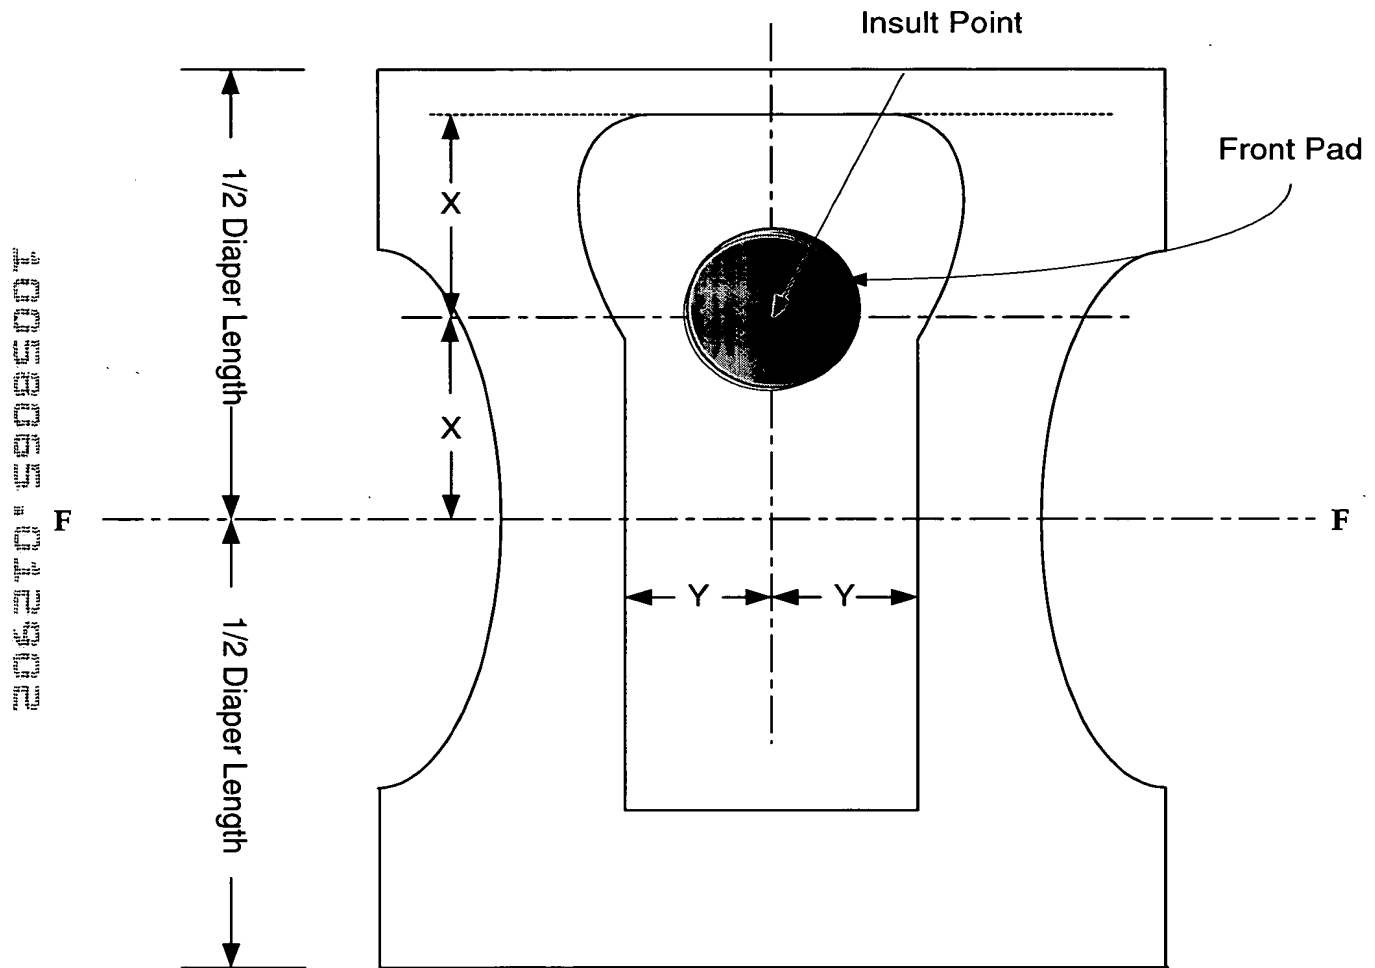


FIG. 4

2025065-012900

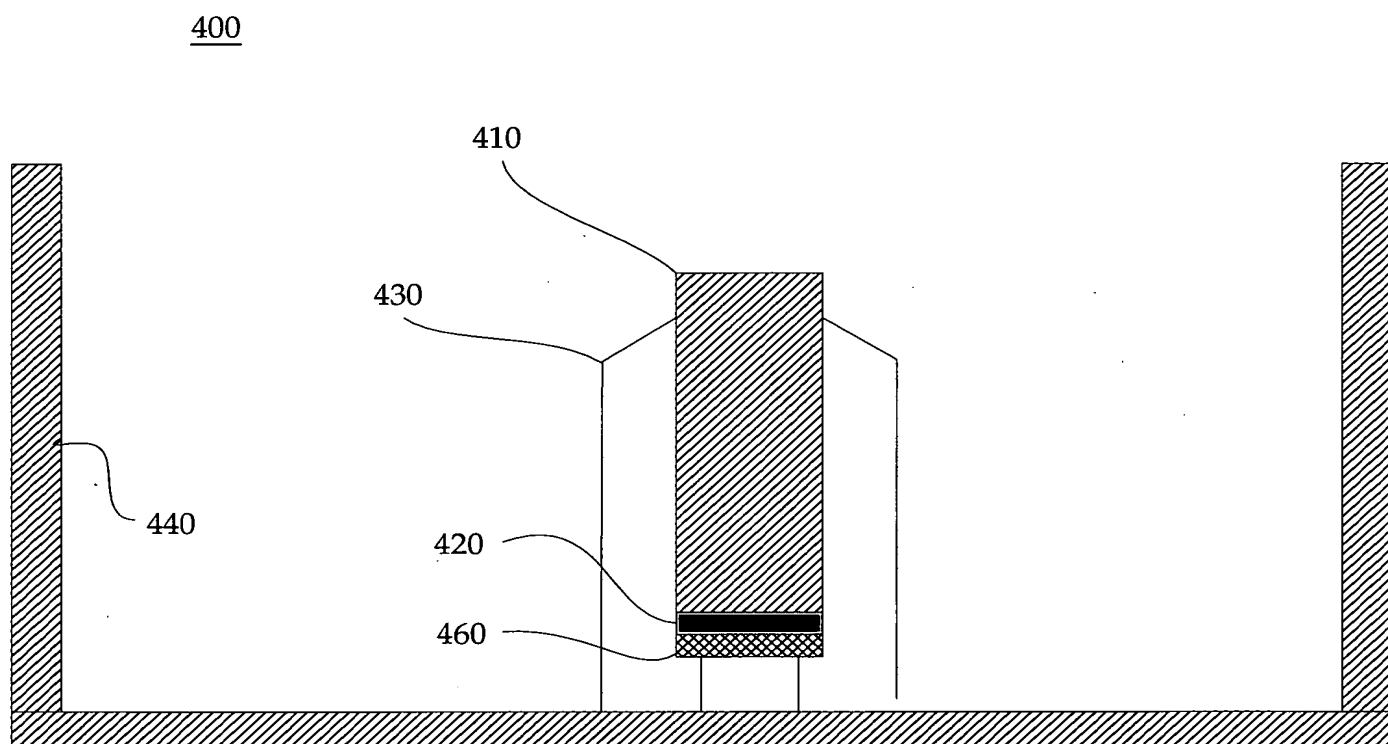
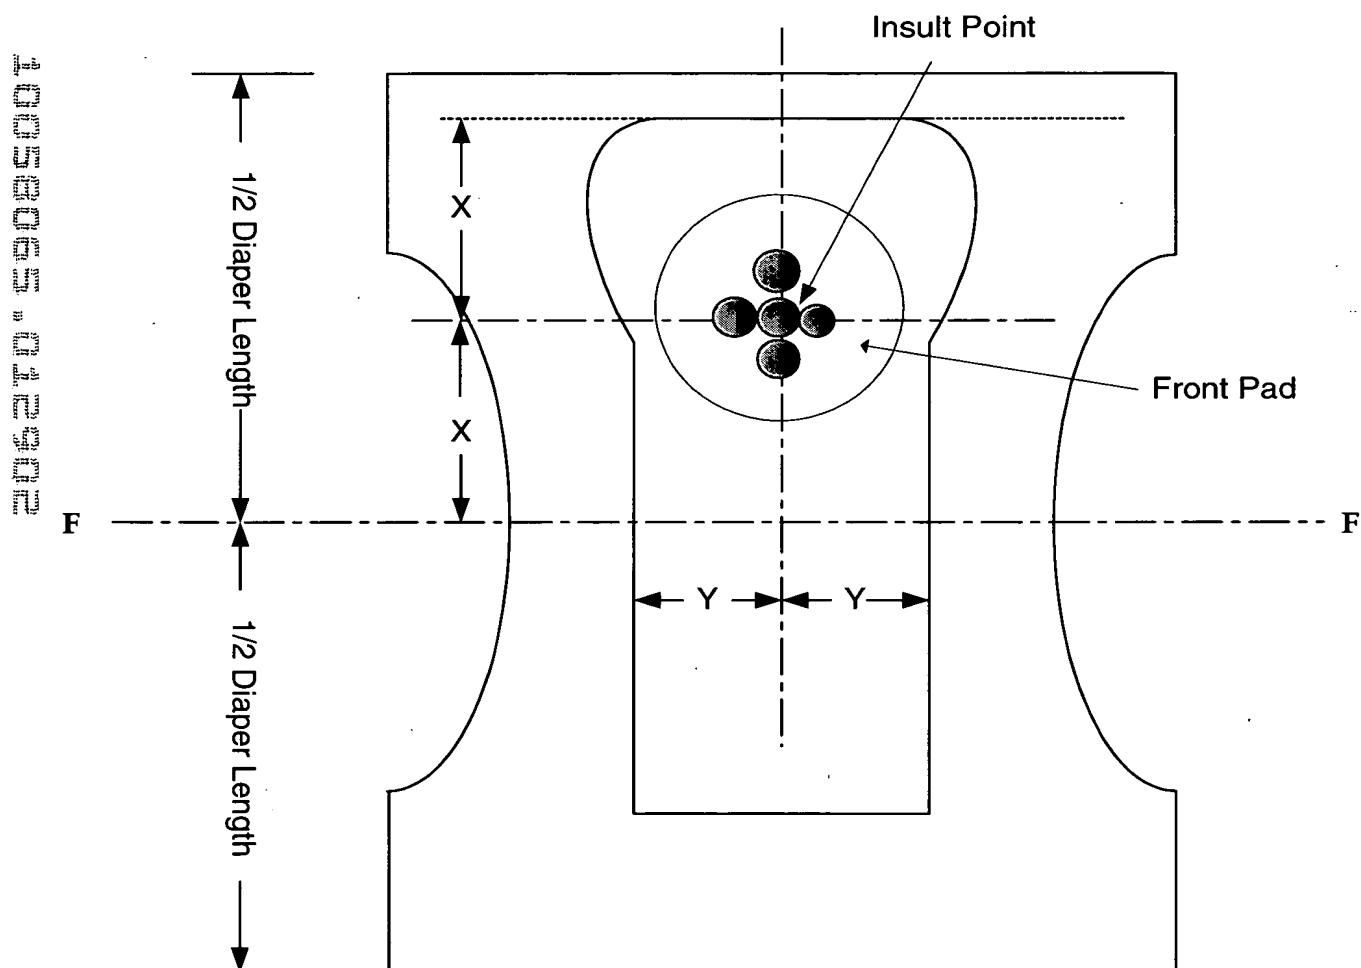


FIG. 5



# TOTAL FRONT PAD CAPACITY v. Urine Leakage

(1.0% NaCl Solution, 10 minutes exposure, 0.5 psi restraining pressure)

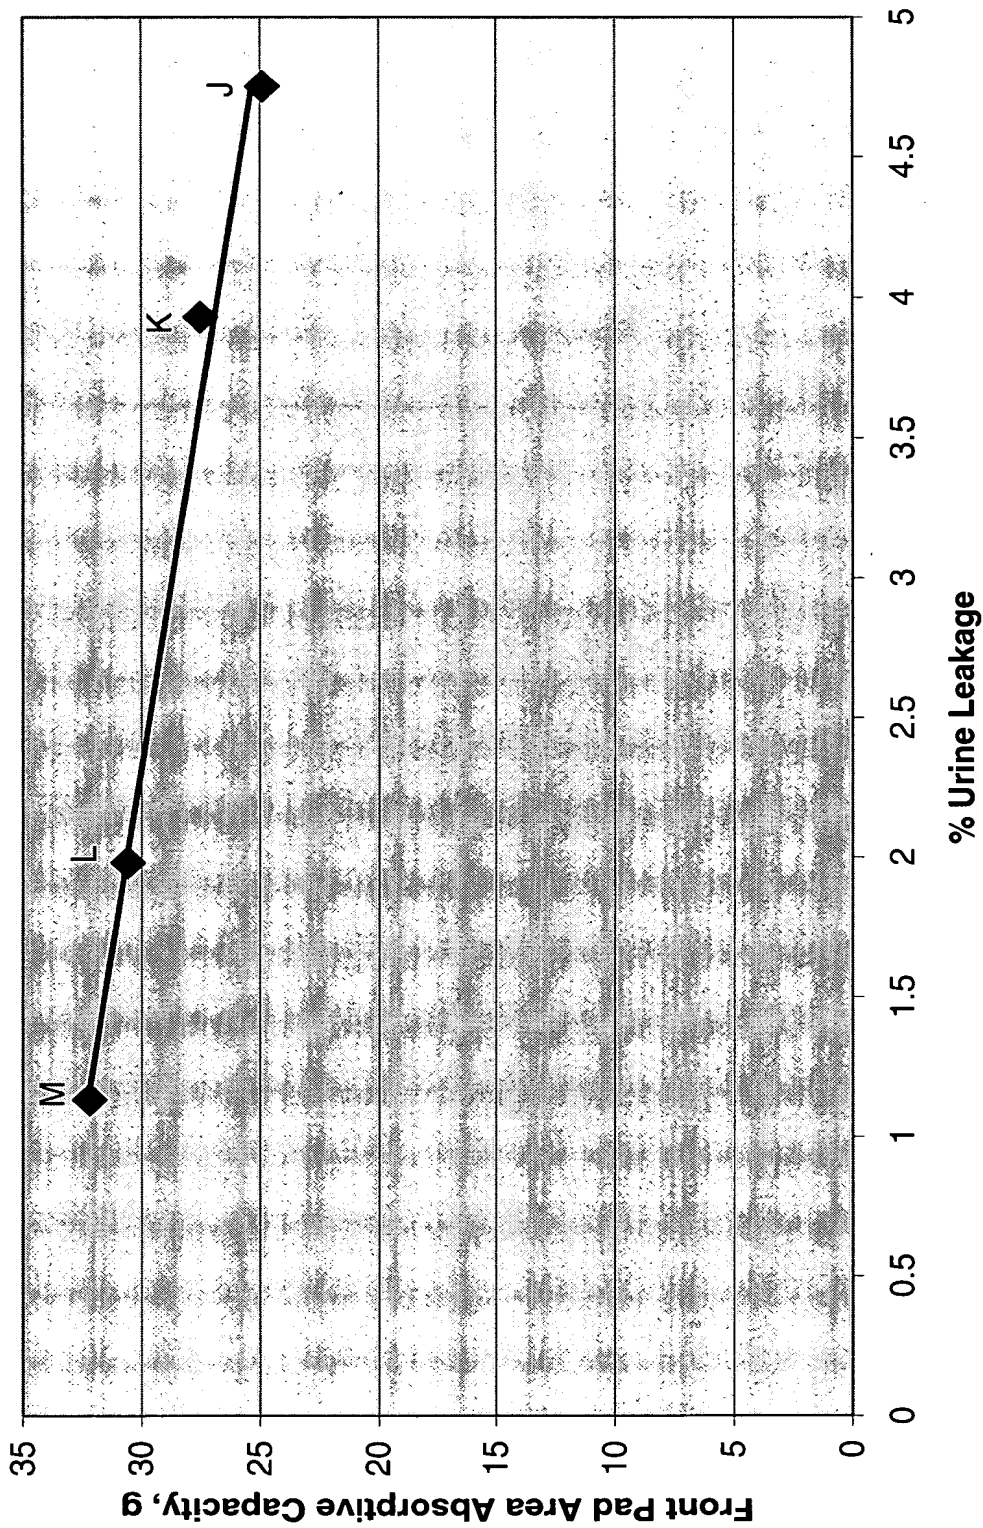


FIG. 6